



Separation, Analysis and Validation of Metal Ions in Aqueous Samples Using Capillary Electrophoresis

Aron Hailemichael^{1*}, Andrew Martin Crouch², Arumugam Manohar¹
and Medhanie Afewerki¹

¹Department of Chemistry, College of Science, Eritrea Institute of Technology, Mei-Nefhi,
P.O.Box 12676, Eritrea.

²Department of Chemistry, University of Stellenbosch, Private Bag X1, Matieland, 7602, South Africa.

Authors' contributions

This work was carried out in collaboration among all authors. Authors AH and AMC designed the study, performed the statistical analysis, wrote the protocol and wrote the first draft of the manuscript. Authors AM and MA managed the analyses of the study and the literature searches. All authors read and approved the final manuscript.

Article Information

DOI: 10.9734/IRJPAC/2019/v18i430098

Editor(s):

(1) Dr. Farzaneh Mohamadpour, Department of Organic Chemistry, University of Sistan and Baluchestan, Iran.

Reviewers:

(1) Jolanta Flieger, Medical University of Lublin, Poland.

(2) Pardon Kusaziwa Kuipa, Lupane State University, Zimbabwe.

(3) Ronald Bartzatt, University of Nebraska, USA.

Complete Peer review History: <http://www.sdiarticle3.com/review-history/49066>

Received 28 February 2019

Accepted 13 May 2019

Published 29 May 2019

Original Research Article

ABSTRACT

Capillary electrophoresis (CE) has been developed as one of the powerful separation techniques for the analysis of inorganic and organic ions in complex matrices in the recent past. In aqueous samples, most of the inorganic ions are having weak absorption profiles in the UV-Vis region of the spectrum. These low absorption profile ionic species are commonly detected by indirect UV absorbance with the addition of an absorbing co-ion (chromophore) into the electrolyte. The inorganic cations oftenly require an additional complexing agent to selectively alter their similar mobilities and proper separation. The indirect detection at 214 nm was performed with α -hydroxyisobutyric acid (α -HIBA)-4-aminopyridine background electrolyte (BGE) that has a characteristic absorbance at 214 nm. The BGE was applied for the separation, analysis, and validation of metal ions in water samples. The metal ions such as K^+ , Na^+ , Ca^{2+} , Mg^{2+} , Mn^{2+} , Fe^{2+} , Cd^{2+} , Pb^{2+} , Ni^{2+} and Zn^{2+} were separated successfully in this study. Also, the effect of electrolyte pH, applied voltage and injection time for the separation of cations was investigated.

*Corresponding author: E-mail: hharmon2007@gmail.com;

Keywords: Water analysis; background electrolyte composition; complexation; cations.

1. INTRODUCTION

Inorganic and organic ions released to the environment may cause risks to the balance of nature. The ions appear to contaminate the water supply systems (surface water and drinking water) and are found as concentrates in ecological systems [1]. Environmental pollutants are a significant hazard to human health, among them trace elements can be beneficial or harmful effects depending on their concentration and chemical form in the living organisms. In addition to the common elements (sodium, calcium, magnesium etc.), a number of trace elements (selenium, zinc, molybdenum, manganese, etc.) are considered essential with specific biological functions at relatively low levels. However, when present in excess, these elements can be harmful [2,3].

Detection of cations and anions can be performed using direct and indirect modes of detection. Direct refers to an analytical signal related directly to the chemical or physical properties of each cation or anion (for example, the energy of emitted X-rays). Indirect mode of detection refers to signals that are non-specific for the cation or anion and are obtained from a transformed species containing the cation or anion (for example, the UV-Vis spectrum of complexed metal ion) or from a species containing no cation or anion from the sample (for example, the signal from the background electrolyte in indirect UV-Vis or fluorescence detection).

The indirect mode of detection requires UV-absorbing species (chromophore) and complexing reagents. In cation analysis, a complexing ligand must be added to the background electrolyte to provide adequate separation by enhancing the difference in mobility among the cations. In addition, the separation buffer or background electrolyte contains a chromophore that provides a background level of absorption at the detection wavelength. The chromophore is displaced by the analyte ions and a decrease in the background absorption is measured when the analyte is in the detector window [4]. In this paper we report on α -hydroxyisobutyric acid (α -HIBA)-4-aminopyridine background electrolyte (BGE) employed for the separation, analysis, and validation of the cations K^+ , Na^+ , Ca^{2+} , Mg^{2+} , Mn^{2+} , Fe^{2+} , Cd^{2+} , Pb^{2+} , Ni^{2+} and Zn^{2+} . In addition,

we have also included the investigation pertaining to the effect of electrolyte pH, applied voltage and injection time for the separation of cations.

2. MATERIALS AND METHODS

2.1 Instrumentation

The CE analysis was performed on a Prince Technologies (Emmen, Netherlands) capillary electrophoresis system equipped with a power supply (0 - \pm 35 kV) and UV detector (PU 4225 UV detector, Philips) with wavelength of 190-820 nm. Fused-silica capillaries (Polymicro Technology, Phoenix, AZ, USA) of 75 μ m I.D., (360 μ m O.D) and 108.5 cm long (96.5 cm effective length) were used. The applied voltage was +25 kV. Samples were introduced into the capillary by the hydrodynamic mode (50 mbar) for 12-24 s. Data acquisition and analysis (DAX) software from Prince Technologies was used for the control of instrument settings. All experiments were conducted at 25°C. The current was monitored for all evaluated back ground electrolytes and was in the range of 8 to 11 μ A.

2.2 Materials

Manganese, Cadmium, Zinc and Lead (all Spectro sol grades) were obtained from Fluka (Buchs, Switzerland). $MgCl_2 \cdot 6H_2O$, Copper (Spectro Sol), Nickel (Spectro Sol) were obtained from Merck (Darmstadt, Germany). α -HIBA (98%), 4-aminopyridine (98%) and H_3PO_4 (85%) were from Aldrich (Steinheim, Germany). NaOH (99%) and HCl (99%) were from Riedel-deHaen (France). $CaCl_2 \cdot 2H_2O$ (97%) and $FeSO_4 \cdot 7H_2O$ (97%) were from NT laboratory supplies (Johannesburg). NaCl (99%) and KCl (99%) were from PAL Chemicals.

2.3 Samples

The standard aqueous samples were prepared and stored in polyethylene containers and acidified and then kept in refrigerator at +4 °C. For CE measurements all samples were first screened with CE and their concentration were estimated. When the peak resolution was not satisfactory (high ionic strength) or the ion zones were distorted, the samples were diluted with ultra purified water (Milli-Q water, prepared in the purification unit) and filtered through 0.45 μ m membranes to achieve better separation for quantification. The samples were not

manipulated by pH adjustment or complexation, because we wanted to analyse them by simulating the natural water conditions as closely as possible.

2.4 Conditioning of the Capillary

New capillaries were conditioned by purging with 1M NaOH solution (30 min), Milli-Q water-ultra pure water (30 min) and running electrolyte (30 min) and the sample was injected with the appropriate method. Capillaries were washed after every change of electrolyte with a 5 min rinse of 1 M NaOH solution and then with water and the appropriate electrolyte.

2.5 Standard Mixtures

Metal cation standard solutions were obtained by dilution in Milli-Q water from 1000 mg/L stock solutions. The mixtures for capillary electrophoretic studies were prepared from the stock solutions to the concentrations needed. All mixtures were ultrasonicated daily before use. The stock solutions were kept in a refrigerator, at 4°C.

2.6 Calibration Solutions

A calibration curve was prepared with 5 mg/L, 25 mg/L, 50 mg/L, 100 mg/L and 200 mg/L concentrations by measuring 25 µL, 125 µL, 250 µL, 500 µL and 1000 µL respectively of each cation in 5 mL volumetric flasks and diluting with Milli-Q water to the mark. The calibration curves were measured only at the ranges suitable for real samples. The linear ranges of each ion were measured at specified injection time.

3. RESULTS AND DISCUSSION

The separation of metal ions was accomplished using different complexing agents and UV-absorbing species. The most important optimization parameter for the separation of cationic compounds is the choice of a suitable background electrolyte. In this study, α -hydroxyisobutyric acid and 4-aminopyridine (1:1) BGEs were used. The different concentrations of complexing agent can change the migration order of metal ions since metal complexes have different stability thus mobility at different concentration of complexing agent.

3.1 Separation of Metal Ions

In the separation method, α -hydroxyisobutyric acid and 4-aminopyridine (1:1) were used as the

complexing agent and background electrolyte respectively for the separation of a mixture of ions. A mixture of 10 metal ions could be separated efficiently using 4-aminopyridine (Fig. 1a). All the peaks were completely resolved. Using this method it was possible to detect Cd^{2+} and Pb^{2+} ions. Table 1 shows the quantitative data for migration time, peak areas and corrected peak areas of the metal ions in the standard mixture. Capillary electrophoresis has comparative advantages over AAS, due to: high speed of analysis, high separation efficiency, low consumption of electricity and samples, method robustness and simplicity, good tolerance to sample matrix.

Higher reproducibility was obtained over three runs (within runs) as shown in Fig. 1b and the reproducibility decreases over three runs (between runs), in this plot a drift to some degree in migration time (especially with that of Ni^{2+} and Zn^{2+}) was observed in Fig. 1c. This may be due to capillary buffer temperature change, buffer evaporation and low stability of voltage over time that was also seen with other runs. Capillary electrophoresis suffers from instability and irreproducibility of migration times and peak areas with time [5].

3.2 The Analysis of Synthetic and Environmental Samples

3.2.1 Analysis of synthetic samples

α -Hydroxyisobutyric acid-4-amino pyridine background electrolyte was chosen for the analysis of real samples since all 10 metals could be analysed. α -Hydroxyisobutyric acid is a widely used complexing agent since it complexes with a large number of metal ions [6] and contains suitable binding groups (carboxyl, hydroxyl) [7].

A high concentration of α -hydroxyisobutyric acid was used to decrease the electroosmosis flow (EOF) [8] and enhance the resolution. An increase in buffer conductivity and running current resulted in a significant increase in the baseline noise and markedly decreased the analyte peak response [9]. Optimum injection time was used to reduce overlap resulting from electro migration dispersion that causes a broad peak. The more the concentration of the sample component, the more pronounced is this dispersion and therefore the broader the peak [10]. The pH, the injection time and the separation voltage were the main factors affecting the separation of metal ions [11]. The

effect of pH, applied voltage and injection on peak area and migration time has been studied.

3.2.2 Effect of pH of the background electrolyte

Buffer pH has much influence on the separation selectivity of metal and controls the improvement of resolution of complexes [12,13]. The electroosmosis flow (EOF) decreases with a decrease in pH [14,15] owing to a reduced dissociation of surface silanol groups. A decrease in the pH of BGE results in an increase in the difference of the migration times between two neighbouring cations. Changing the pH affects the selectivity and thus the peak area. A pH range between 3 - 6.5 has been studied. Fig. 2 shows a plot of peak area as a function of pH.

A decrease in pH results in an increase in peak area. The increased peak responses are caused by a decreased migration velocity of the sample zone through the detector because peak area is

inversely related to the migration velocity [16,17, 18]. At pH 4.5 the largest peak area response, and consequently the highest sensitivity, were obtained for the cations. At pH below 4.5 a high noise and distortion in background was observed. Likewise, cations like, Mg^{2+} , Pb^{2+} and Zn^{2+} were not seen at pH lower than 4.5. This is because of the distortion of buffer solution and the complexes formed are not stable.

3.2.3 Effect of applied voltage

The increase in the applied voltage increases in the velocity of the ion and consequently its migration time. The relation between velocity of the ion (V), migration time (μ) and the applied voltage (E) [19] is given by:

$$V = \mu E$$

The plot of the migration time as a function of applied voltage is given in Fig. 3.

Table 1. The migration time, peak area and corrected peak area of metal ions at a concentration of 10 ppm (n = 6)

Metal ion	Migration time, min (RSD)	Peak area, (RSD)	Corrected peak area, (RSD)
K^+	7.99(±1.74%)	3.65E-05(±6.74%)	4.57E-06(±6.50%)
Ca^{2+}	10.04(±2.79%)	3.87E-05(±7.13 %)	3.86E-06(±5.26%)
Na^+	10.41(±2.83%)	6.47E-05(±4.85%)	6.22E-06(± 4.72%)
Mg^{2+}	10.77(±3.03%)	3.43E-05(±7.64%)	3.19E-06(±6.48%)
Mn^{2+}	11.07(±3.16%)	0.000138(±8.05%)	1.25E-05(±5.44%)
Fe^{2+}	11.38(±3.36%)	2.01E-05(±4.85%)	1.76E-06(±3.70%)
Cd^{2+}	11.69(±3.51%)	7.20E-05(±5.86%)	6.17E-06(±2.97%)
Pb^{2+}	11.83(±3.81%)	1.67E-05(±12.04%)	1.42E-06(±11.83%)
Ni^{2+}	12.023(±3.84%)	1.32E-04(±8.46%)	1.10E-05(±5.72%)
Zn^{2+}	12.21(±3.94%)	1.20E-04(±8.36%)	9.85E-06(±5.27%)

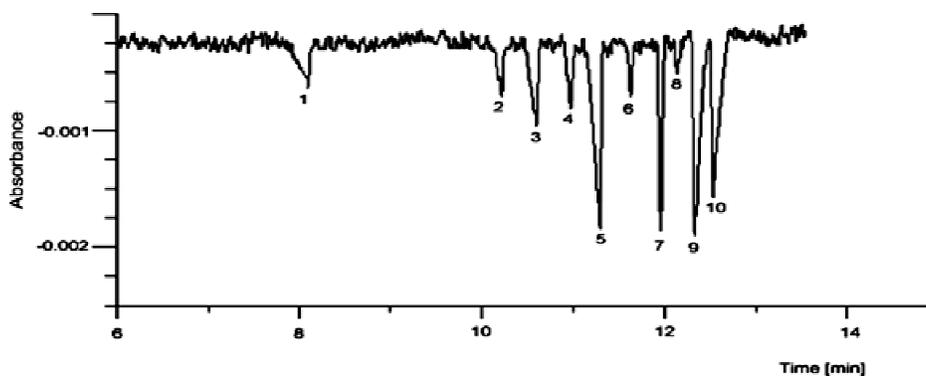


Fig.1a Electrophoretic separation of 10 metal ions. Carrier electrolyte, 10 mM 4-amino pyridine and 6.5 mM α -hydroxylisobutyric acid(1:1) (pH 4.5); hydrodynamic injection 18 s; voltage, 25 kV; wavelength, 214 nm. Peaks according to sequence: 1= K^+ , 2 = Ca^{2+} , 3 = Na^+ , 4 = Mg^{2+} , 5 = Mn^{2+} , 6 = Fe^{2+} , 7 = Cd^{2+} , 8 = Pb^{2+} , 9 = Ni^{2+} , 10 = Zn^{2+}

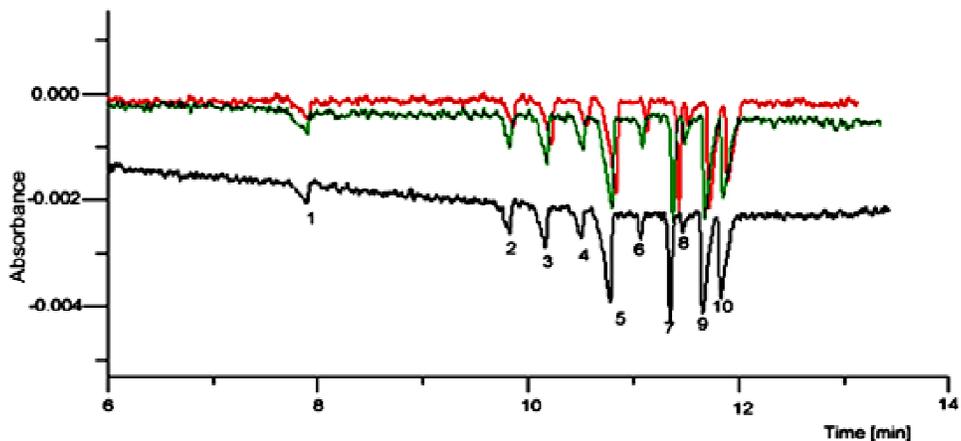


Fig.1b. The reproducibility (within runs) of metal ions over three runs using the same experimental conditions as in Fig. 1a. Peaks according to sequence: 1 = K^+ , 2 = Ca^{2+} , 3 = Na^+ , 4 = Mg^{2+} , 5 = Mn^{2+} , 6 = Fe^{2+} , 7 = Cd^{2+} , 8 = Pb^{2+} , 9 = Ni^{2+} , 10 = Zn^{2+}

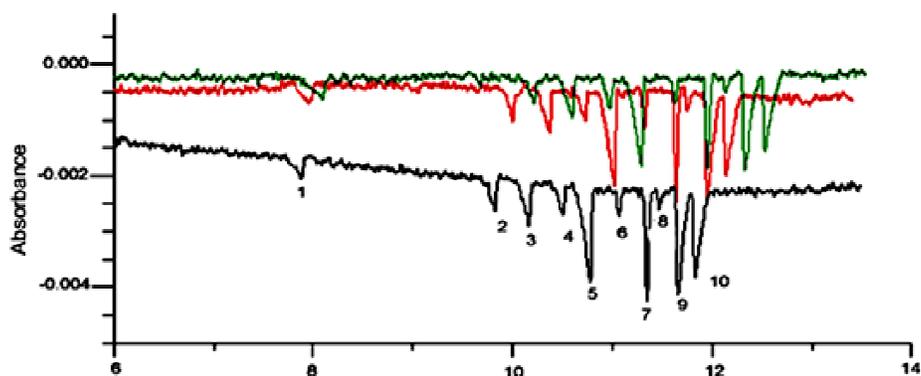


Fig.1c. The reproducibility of metal ions over three runs (between runs) using the same experimental conditions as in Fig. 1a. Peaks according to sequence: 1 = K^+ , 2 = Ca^{2+} , 3 = Na^+ , 4 = Mg^{2+} , 5 = Mn^{2+} , 6 = Fe^{2+} , 7 = Cd^{2+} , 8 = Pb^{2+} , 9 = Ni^{2+} , 10 = Zn^{2+}

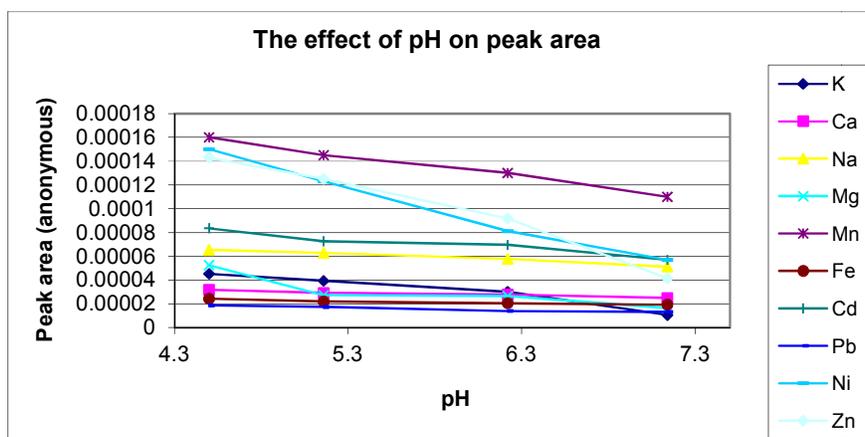


Fig. 2. The effect of pH of the background electrolyte on peak area. Experimental conditions are the same as in Fig.1a

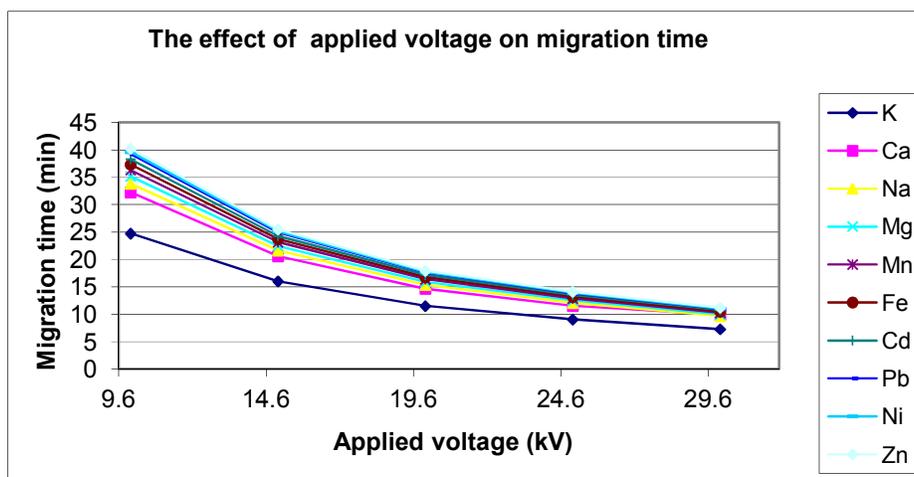


Fig. 3. The effect of applied voltage on migration time. Experimental conditions are the same as in Fig.1a

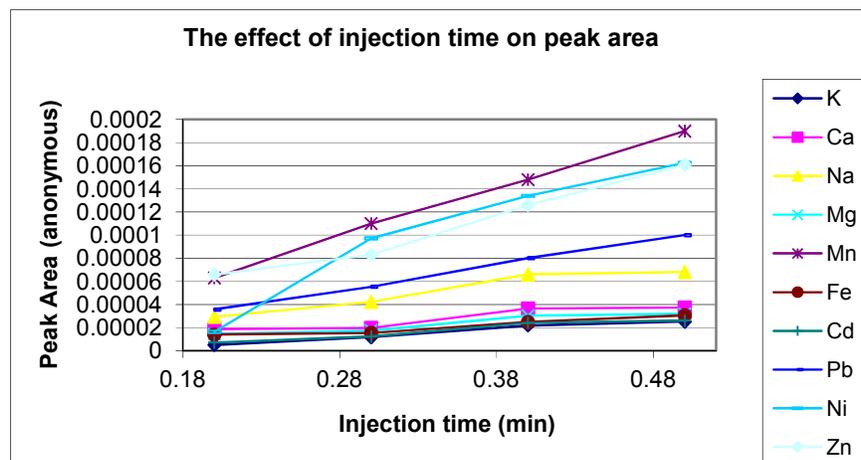


Fig. 4. The effect of injection time on peak area. Experimental conditions are the same as in Fig. 1a

A change in the applied voltage has direct effect on the migration time. The migration time between the neighbouring cations changes when the applied voltage changes from 10 to 30 kV. From the above considerations, a positive voltage of 25 kV was selected for further experiments.

3.2.4 Injection time

The signals obtained were, in general, proportional to the injection time for metals investigated. However, peak broadening was found to occur at long injection time, leading to poor separation [20,21]. The effects of varying injection time to 0.2, 0.3, 0.4 and 0.5 min was studied. High injection time was used since the

sensitivity of the instrument is low. At higher injection time the peak area was increased. Therefore, in this study, 0.3 min for metal separation and 0.2 min for the calibration curve area was used to reduce overlapping. The plot of peak area versus injection time is shown in Fig. 4.


3.2.5 Validation of the method

3.2.5.1 Limit of detection (LOD)


Table 2 shows with hydrodynamic injection for 24 s, at pH 4.5, with respect to each metal ion the following LOD was found. Lower limits of detection was obtained by injecting greater volumes, but at the expense of peak efficiency [22]. A higher limit of detection LOD was obtained for Ca²⁺.

Table 2. The limit of detection of metal ions (ppm)


Cation	LOD	Cation	LOD
K ⁺	3.0	Fe ²⁺	3.0
Na ⁺	2.5	Cd ²⁺	1.0
Ca ²⁺	0.5	Pb ²⁺	3.0
Mg ²⁺	2.5	Ni ²⁺	1.0
Mn ²⁺	1.0	Zn ²⁺	1.0

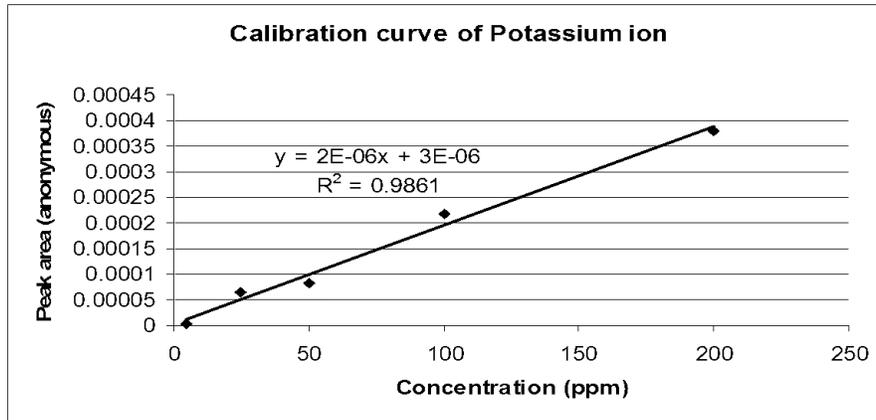


(a)

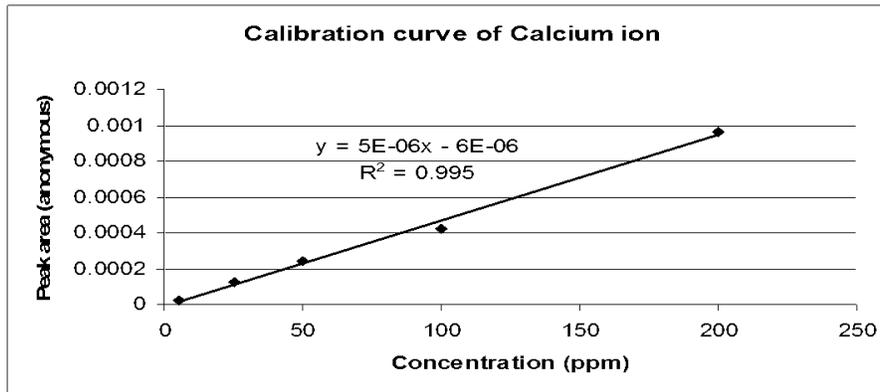

(b)

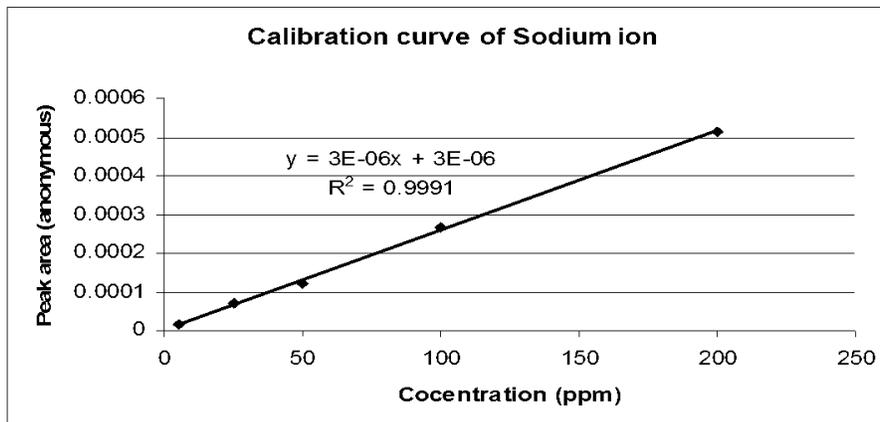

(c)

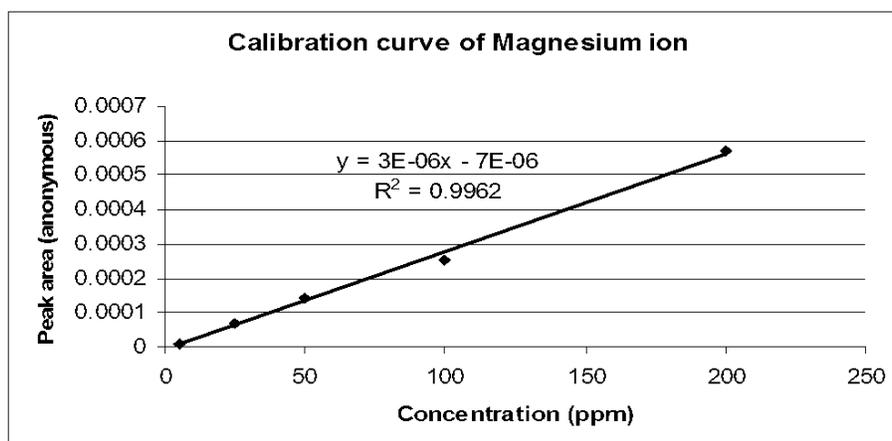

(d)

Fig. 5. Calibration curve of (a) K^+ , (b) Ca^{2+} , (c) Na^+ , (d) Mg^{2+}

The limit of detection of each metal ion was determined by preparing standard solutions of each metal ion to the lowest concentration that can be obtained.

3.2.5.2 Linearity of the calibration line

Standard solutions containing 5, 25, 50, 100, 200 ppm of each mixtures of metal was prepared under the optimised conditions to test the linearity of the response for the metals under the conditions of indirect detection. Five injections were performed at each concentration level. Analytical calibration lines were calculated based on the measurement of the peak areas. Regression values greater than 0.9861 were obtained. The regression value for K^+ was low due to its small peak. The calibration curve for base metal ions is given in Fig. 5.

4. CONCLUSION

Different methods have been developed for the separation, analysis, and validation of metal ions in aqueous samples using capillary electrophoresis. The α -hydroxyisobutyric acid (α -HIBA)-4-aminopyridine background electrolyte (BGE) was effective since it results in for the detection of more number of metal ions. Using α -HIBA as complexing agent and 4-aminopyridine as UV-absorbing compound was the most efficient for the successful determination of all of metal ions. The potential of the method for quantitative and qualitative analysis of metal ions in complex matrix in environmental water sample is presented.

COMPETING INTERESTS

Authors have declared that no competing interests exist.

REFERENCES

1. Sir en H, Vantsi S. Environmental water monitoring by capillary electrophoresis and result comparison with solvent chemistry techniques. *J. Chromatogr. A.* 2002;957: 17-26.
2. Song L, Xu Z, Kang J, Chen J. Analysis of environmental pollutants by capillary electrophoresis with emphasis on micellar electrokinetic chromatography. *J. Chromatogr A.* 1997;780:297-328.
3. Liu YM, Cheng JK. Elemental speciation analysis in capillary electrophoresis. *Electrophoresis.* 2003;24:1993-2012.
4. Carla Vogt. *J. Anal. Chem.* 2001;370:316-318.
5. Altria KD, Frake P, Gill I, Hadgett T, Rudd DR. Validated capillary electrophoresis method for the assay of a range of basic drugs. *J. Pharm. Biomed. Anal.* 1995;13: 951-957.
6. Fung YF, Lau KM. Determination of trace metals by capillary electrophoresis. *Electrophoresis.* 2001;24:2192-2200.
7. Pacakova V, Coufal P, Stulik K. Capillary electrophoresis of inorganic cations. *J. Chromatogr. A.* 1999;834:257-275.
8. Scarcella D, Tagliaro F, Turrina S, Manetto G, Marigo M. Optimization of a simple method for the chiral separation of

- phenethylamines of forensic interest based on cyclodextrin complexation capillary electrophoresis and its preliminary application to the analysis of human urine and hair. *Forensic Science International*. 1997;89:33-46.
9. Yang Q, Jimidar M, Hamoir TP, Smeyers-Verbeke J, Massart DL. Determination of alkali and alkaline earth metals in real samples by capillary ion analysis. *J. Chromatogr. A*. 1994;673:275-285.
 10. Foret F, Fanali S, Ossicini L, Bocek P. Indirect photometric detection in capillary zone electrophoresis. *J. Chromatogr. A*, 1989;470:299-308.
 11. Xiong X, Li SYF. Selection and optimization of background electrolytes for simultaneous detection of small cations and organic acids by capillary electrophoresis with indirect photometry. *J. Chromatogr. A*. 1998;822:125-136.
 12. Liu BF, Liu LB, Cheng JK. Analysis of inorganic cations as their complexes by capillary electrophoresis. *J. Chromatogr. A*. 1999;834:277-308.
 13. Timerbaev AR, Semenova OP. Theoretical estimation of capillary zone electrophoresis behaviour of metal complexes using multivariate regression analysis. *J. Chromatogr. A*. 1995;690:141-148.
 14. Weston A, Brown PR, Hackenberg AL, Jandik P, Jones WR. Effect of electrolyte composition on the separation of inorganic metal cations by capillary ion electrophoresis. *J. Chromatogr. A*. 1992; 602:249-256.
 15. Chen HW, Fang ZL. Combination of flow injection with capillary electrophoresis.: Part 5. Automated preconcentration and determination of pseudoephedrine in human plasma. *Analytica Chimica Acta*. 1999;394:13-22.
 16. Fung YS, Lau KM. Development and validation of analytical methodology using capillary electrophoresis for separation and determination of anions in rainwater. *Talanta*. 1998;45:641-646.
 17. Altria DK. LC.GC. 1993;6:164-171.
 18. Yau WP, Chan E, Chiral CE. Separation of warfarin in albumin containing samples. *J. Pharm. Biomed. Anal.* 2002;28:107-123.
 19. Sunada WM, Blanch HW. Polymeric separation media for capillary electrophoresis of nucleic acids. *Electrophoresis*. 1997;18:2243-2254.
 20. Kennedy RT. Bioanalytical applications of fast capillary electrophoresis. *Analytical Chimica Acta*. 1999;400:163-180.
 21. Fung YS, Tung HS. Capillary electrophoresis for trace metal ion analysis in environmental studies. *Electrophoresis*. 1999;20:1832-1841.
 22. Padaruskas A, Schwedt G. Capillary electrophoresis in metal analysis: Investigations of multi-elemental separation of metal chelates with aminopolycarboxylic acids. *J. Chromatogr. A*. 1997;773:351-360.

© 2019 Hailemichael et al.; This is an Open Access article distributed under the terms of the Creative Commons Attribution License (<http://creativecommons.org/licenses/by/4.0>), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

Peer-review history:

The peer review history for this paper can be accessed here:
<http://www.sdiarticle3.com/review-history/49066>